1412i/1314i Photoacoustic Gas Monitor

Quick Set-up Guide
BR6021-11

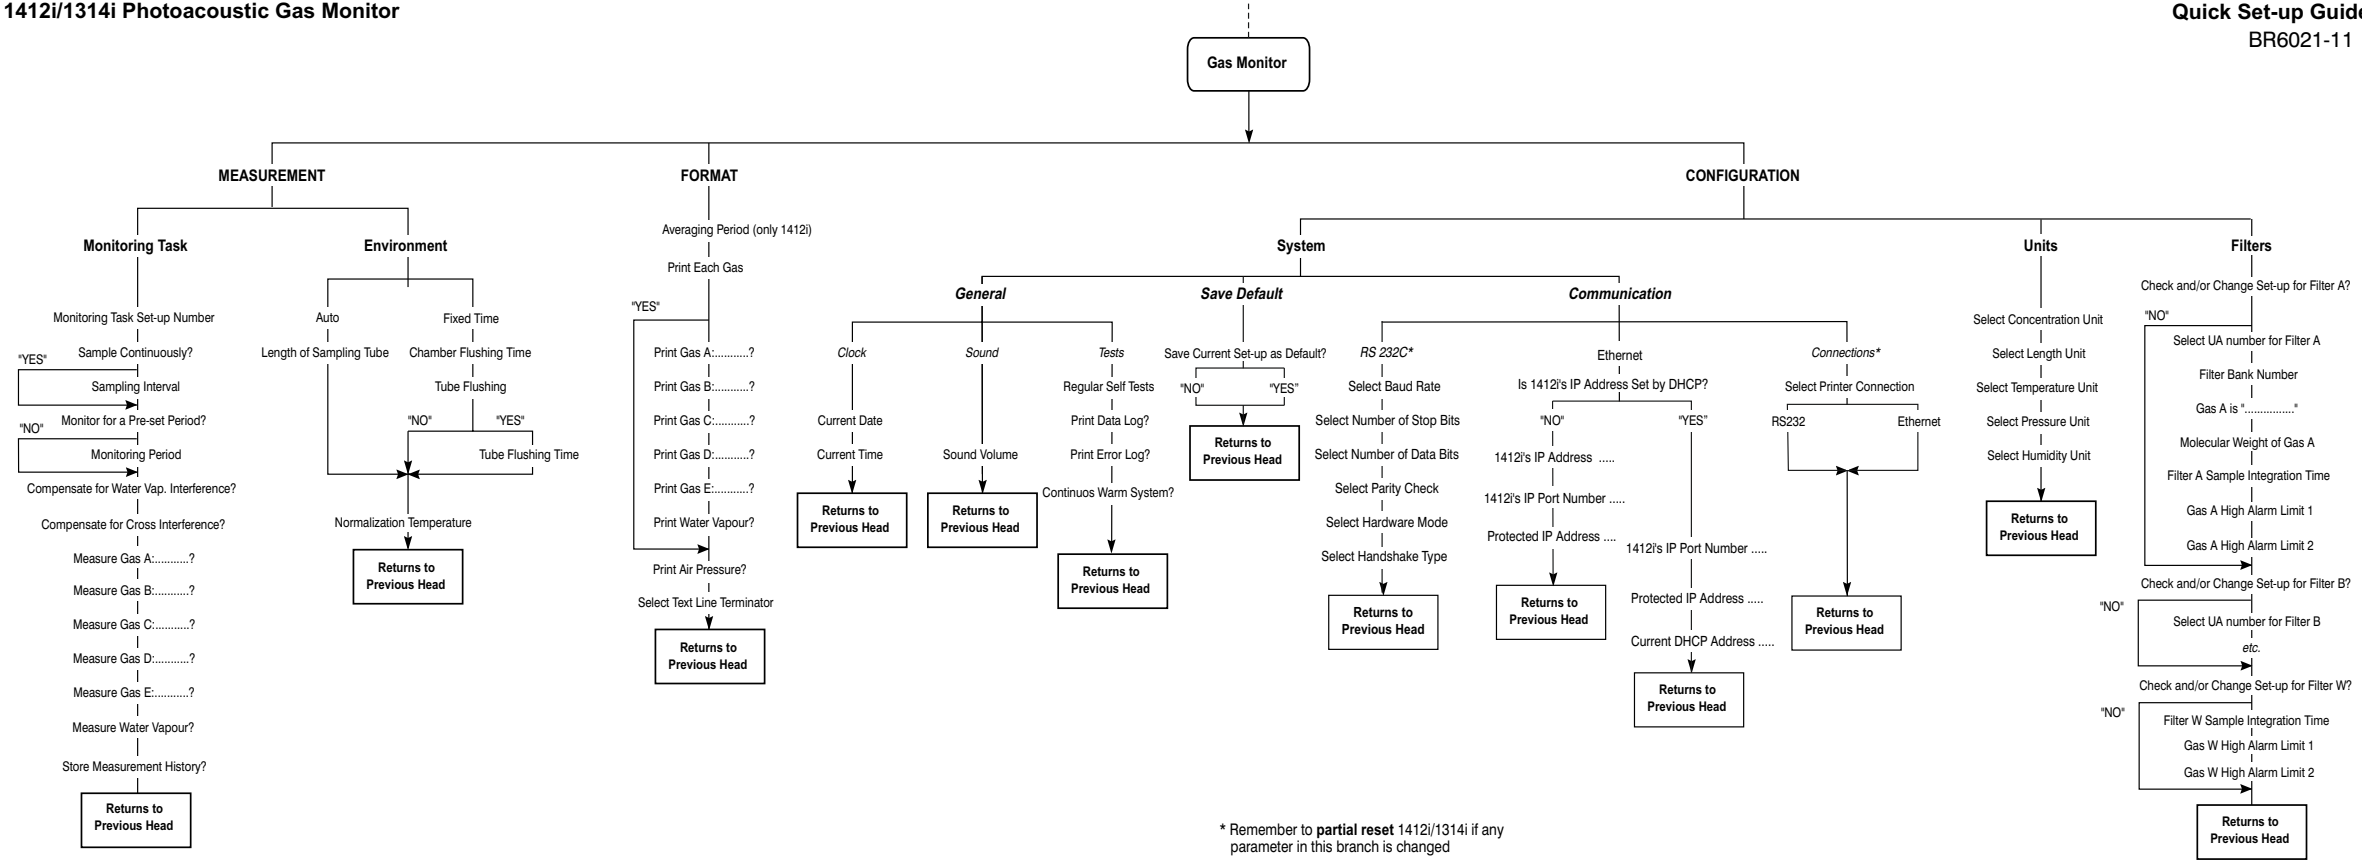

* Remember to **partial reset** 1412i/1314i if any parameter in this branch is changed